

SUPPLEMENTARY MATERIAL TO  
**Highly sensitive, non-enzymatic and precious metal free  
electrochemical glucose sensor based on Ni–Cu/TiO<sub>2</sub> modified  
glassy carbon electrode**

ABDUL RAZIQ, MUHAMMAD TARIQ\*, RIAZ HUSSAIN, MUHAMMAD H.  
MEHMOOD, INAM ULLAH, JAHANGEER KHAN and MAMRIZ MUHAMMAD

National Centre of Excellence in Physical Chemistry University of Peshawar, Peshawar-  
25120, Pakistan

J. Serb. Chem. Soc. 83 (6) (2018) 733–744

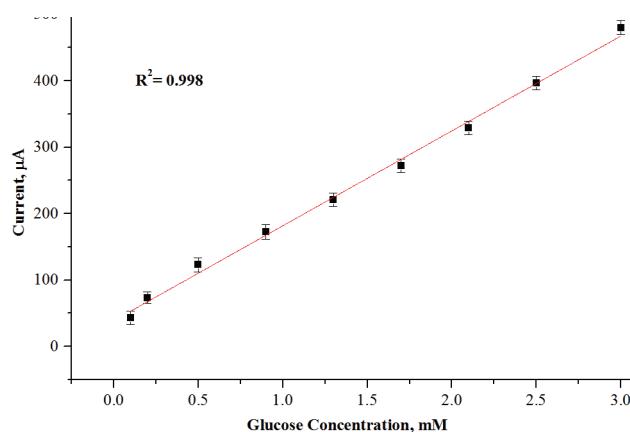


Fig. S-1. Peak current ( $I_p$ ) vs. concentration.

\*Corresponding author. E-mails: dr.muhammadtariq@upesh.edu.pk, tariq\_ftj@yahoo.com

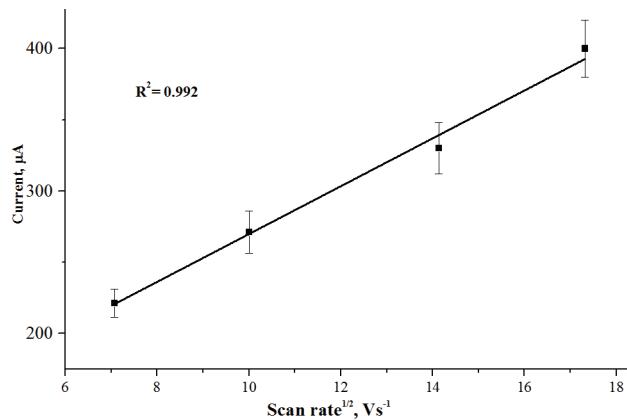


Fig. S-2. Peak current vs. square root of scan rate ( $v^{1/2}$ ).

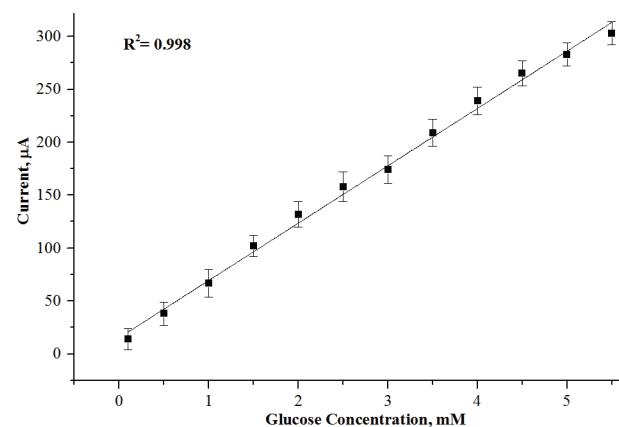


Fig. S-3.  $I_p$  vs. concentration.